

User Guide

4-Channel High Sensitivity (N1) Cartridge Kit (C405105)

A. Specifications

Specification	Description
DNA Sizing Range	20-5,000 bp
L.O.D	5 pg/ μ L
Resolution*	4-10 bp
Sample Number	400 runs**
Shelf Life	4 months

* Best resolution is determined by the 15-622 DNA Size Marker (C109200).

** 100 runs/channel x 4 channels = 400 runs


B. Kit Components and Storage Conditions

Item	Storage Condition
4-Channel High Sensitivity Cartridge (C405105)	4-30°C (Do Not Freeze)
20-1,000 bp Alignment Marker (C109100-500A, 500 μ L)	Short-Term ($\leq$ 3 months): 4-30°C Long-Term ($>$ 3 months): -20°C
Separation Buffer (C104409, 100 mL)	4-30°C
Dilution Buffer (C104408, 30 mL)	4-30°C
Mineral Oil (C104407, 15 mL)	4-30°C

C. Cartridge Unpacking Preparation

The new cartridge must undergo HV check and calibration. Please place 4 tubes of 20 μ L C109100 Alignment Marker at positions AM01, AM04, AM07, and AM10, and follow the instructions provided in the unpacking guide to complete the calibration process.

D. Buffer, Marker, and Sample Preparation

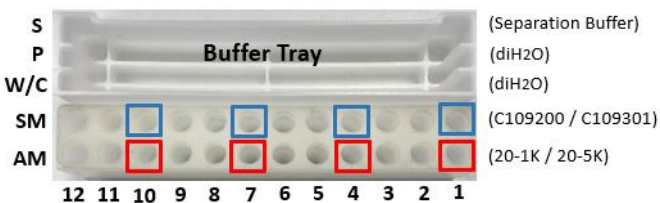


4-Channel position:

- (1) Channel 1 : A1-H1/A2-H2/A3-H3
- (2) Channel 2 : A4-H4/A5-H5/A6-H6
- (3) Channel 3 : A7-H7/A8-H8/A9-H9
- (4) Channel 4 : A10-H10/A11-H11/A12-H12

*All 4 channels will be analyzed simultaneously.

*Sample should be in quadruple number. Otherwise, tubes with dilution buffer should be used.

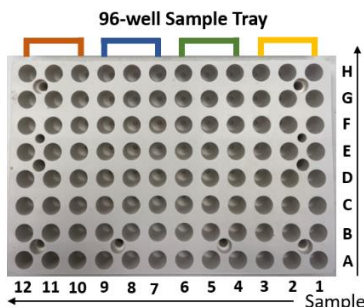

The 4-channel system can be interpreted as 4 individual cartridges. Thus, the sample number should be quadruple.

For example, if 4 samples are assigned at A1, A4, A7, and A10, then 6 samples can be assigned at A1, A4, A7, A10, B1, and B4, with dilution buffer at B7 and B10.

1. Compatible Sample Tubes

Name	Cat. No.	Volume	Image
Micro Vial	C104250	$\geq$ 2 μ L	
0.1 mL PCR Tube	-	$\geq$ 10 μ L	
0.2 mL PCR Tube	-	$\geq$ 20 μ L	
Semi/Non-skirted 96-well Plate*	-	10-20 μ L	

* Recommended 96-well plates: Labcon (3972-520-000), Axygen (PCR-96-FLT-C).

2. Buffer Preparation



Use the droppers to fill the wells. Each well should be 80% full. Overfilling or having droplets left on the dividers will conduct the currents and make it hard to keep track of the changes.

3. Markers Required for Different Size Ranges

- For Sample Size Range from 20 bp to 1,000 bp:
 - 20 bp-1,000 bp Alignment Marker (C109100)
 - 20X diluted** 15-622 bp Size Marker (C109200)
- For Sample Size Range from 20 bp to 5,000 bp:
 - 20 bp-5,000 bp Alignment Marker (C109102)
 - 10X diluted** 50 bp-3,000 bp Size Marker (C109301)

4. Recommended Sample Concentration

Fragmented sample: 10-200 pg/ μ L

- If the fragment sample concentration exceeds 200 pg/ μ L, dilute the sample 10X using 0.5X dilution buffer.


Smear sample (NGS library/cfDNA): 50-1,000 pg/ μ L

- If the fragment sample concentration exceeds 1,000 pg/ μ L, dilute the sample 10X using 0.5X dilution buffer.
- If the sample is eluted in water, add dilution buffer to achieve a sample concentration of either 0.2X or 0.1X dilution buffer condition.


User Guide

4-Channel High Sensitivity (N1) Cartridge Kit (C405105)


E. Software Operation Guide

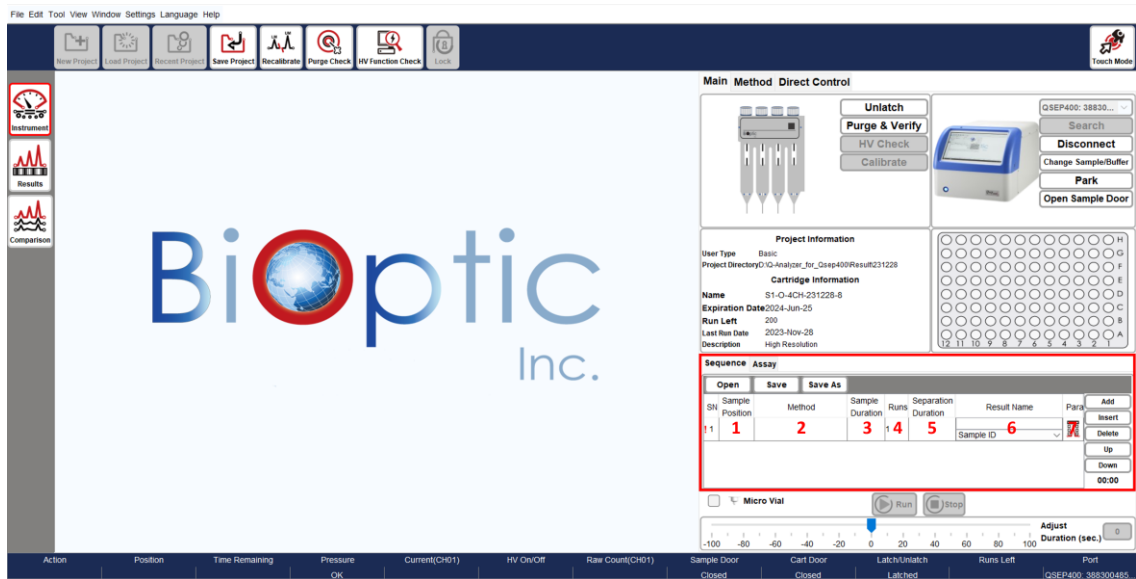

1. Sample Position: Place the sample and select the corresponding position. Input sample information if necessary.

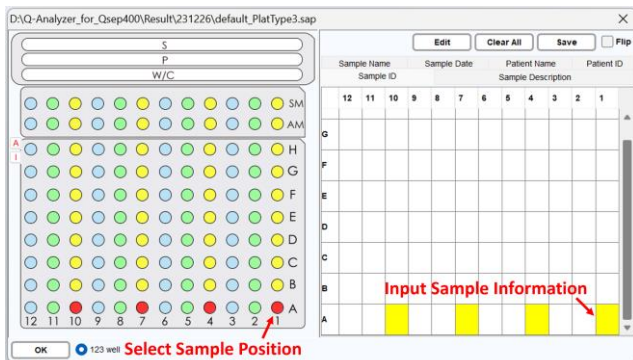

2. Method: Select (a) Alignment Marker and (b) Analytic Method in the Method Selector.

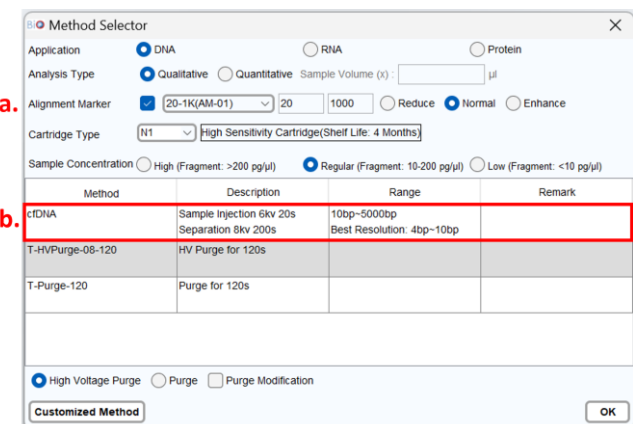

- Adjust injection conditions based on sample concentration.

Sample Concentration	High (2kV, 10s)	Regular (4kV, 10s)	Low (8kV, 10s)
Fragmented DNA	> 200 pg/μL	10-200 pg/μL	< 5 pg/μL
Smear DNA	> 1000 ng/μL	50-1000 pg/μL	< 50 pg/μL

3. Sample Duration: Adjust the sample injection time to increase/decrease injection amount.

- Modify injection conditions based on sample concentration.


4. Runs: Set the repetition time.

5. Separation Duration: Adjust the duration to extend/reduce the separation time.

(Optional)

6. Result Name: Input the result name for the result file.

7. Para: Choose between (a) Reference Marker Table and (b) Create Size Marker for calculation.

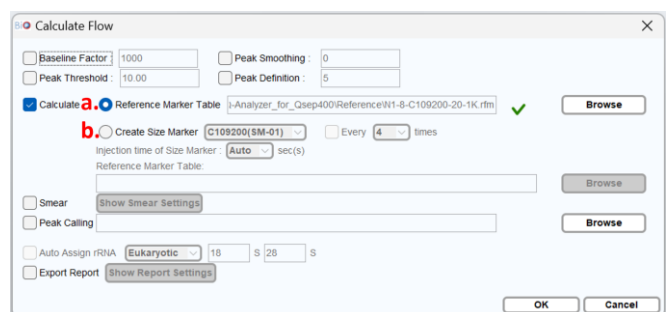

- When using "Create Size Marker" function, select the appropriate size marker you use. For example, "20-1k" is paired with C109200, "20-5k" is paired with C109301.

8. Click "Run" to start the sequence analysis.


User Guide

4-Channel High Sensitivity (N1) Cartridge Kit (C405105)


F. Result & Application

• Alignment Marker & Size Marker Result

20-1K & C109200 15-622 bp Size Marker

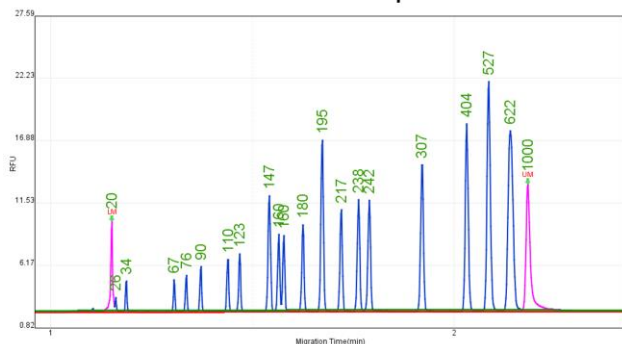


20-5K & C109301 50-3000 bp Size Marker

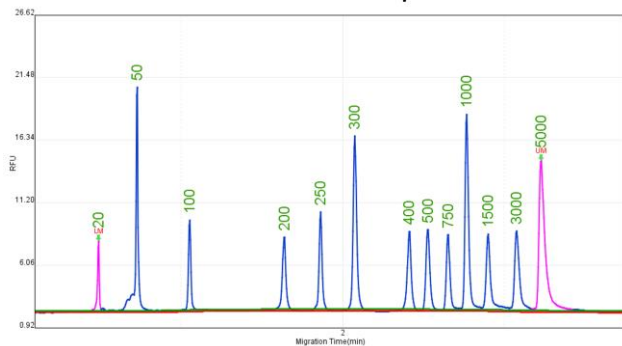

- The 4-channel system can be interpreted as 4 individual cartridges. Therefore, there should be 30-50% individual differences between each of them.

• Cell-Free DNA Validation

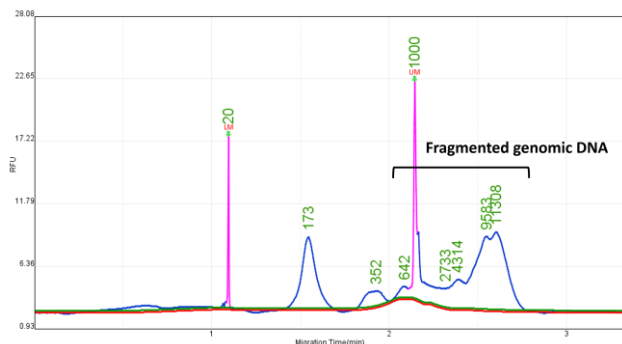

G. Troubleshooting

Before attempting any troubleshooting, ensure that the system is functioning properly and that all operations are following the instructions.

If encountering unstable current during sample injection or separation steps, which may be caused by residues left in the DNA sample after extraction, consider the following solutions:

1. Dilute the sample using dilution buffer.
2. Centrifuge the sample for a period to allow residues to accumulate at the bottom of the tube.
3. Insert a "T-purge-120" method between several sample runs. For example, insert one run of "T-Purge-120" every 5-10 sample runs.

Sequence		Assay							
Open		Save	Save As						
SN	Sample Position	Method	Sample Duration	Runs	Separation Duration	Result Name	Para	Add	
1	A-01.A...	cDNA	20	1	200	Test 1 Sample ID		Insert	
2		T-Purge-120	0	1	0	Sample ID		Delete	
3	B-01.B...	cDNA	20	1	200	Test 2 Sample ID		Up	
								Down	
									01:53

H. Cartridge Disposal

Please wear gloves before discarding the cartridge.



1. Bend the cartridge tip.
2. Open the caps on the gel reservoirs and remove the inner caps.
3. Pour the gel into the chemical waste container.
4. Dispose of the cartridge in the trash bin.

Contact Information:

Company Name: BiOptic Inc.

Address: 5F., No.108, Minquan Rd., Xindian District, New Taipei City 23141, Taiwan

Tel: +886-2-2218-8726, Fax: +886-2-2218-8727, E-mail: service@bioptic.com.tw